



New 100 um 4-laser, 16-color (B3-R3-YG4-V6)

Cytometer:	FACSriaII	User:	Administrator
Cytometer Name:	FACSriaII	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	11/13/2018 2:28:50 PM
Sheath Pressure:	20.00		
Nozzle Size:	100		
Window Extension:	2.00		


488nm Laser
(488nm)
FSC

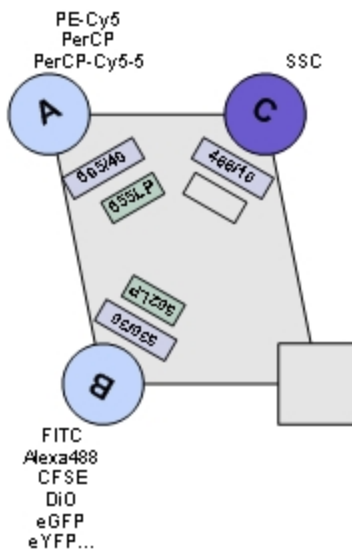


561nm Laser
(561nm)

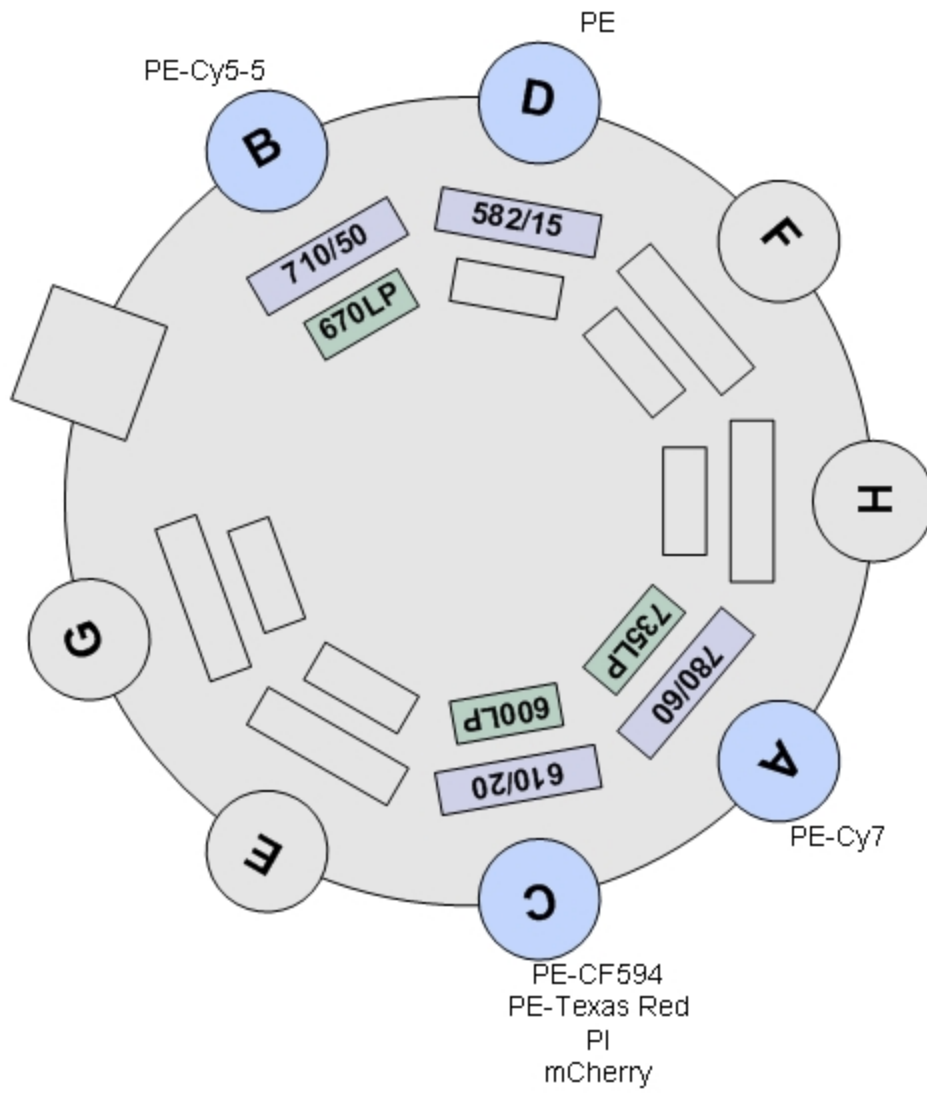

633nm Laser
(633nm)

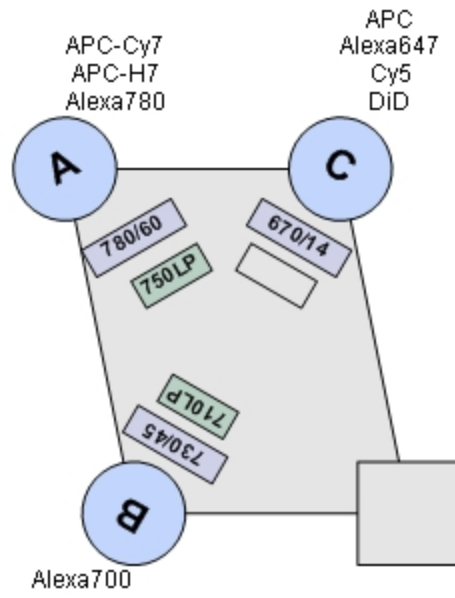

405nm Laser
(405nm)

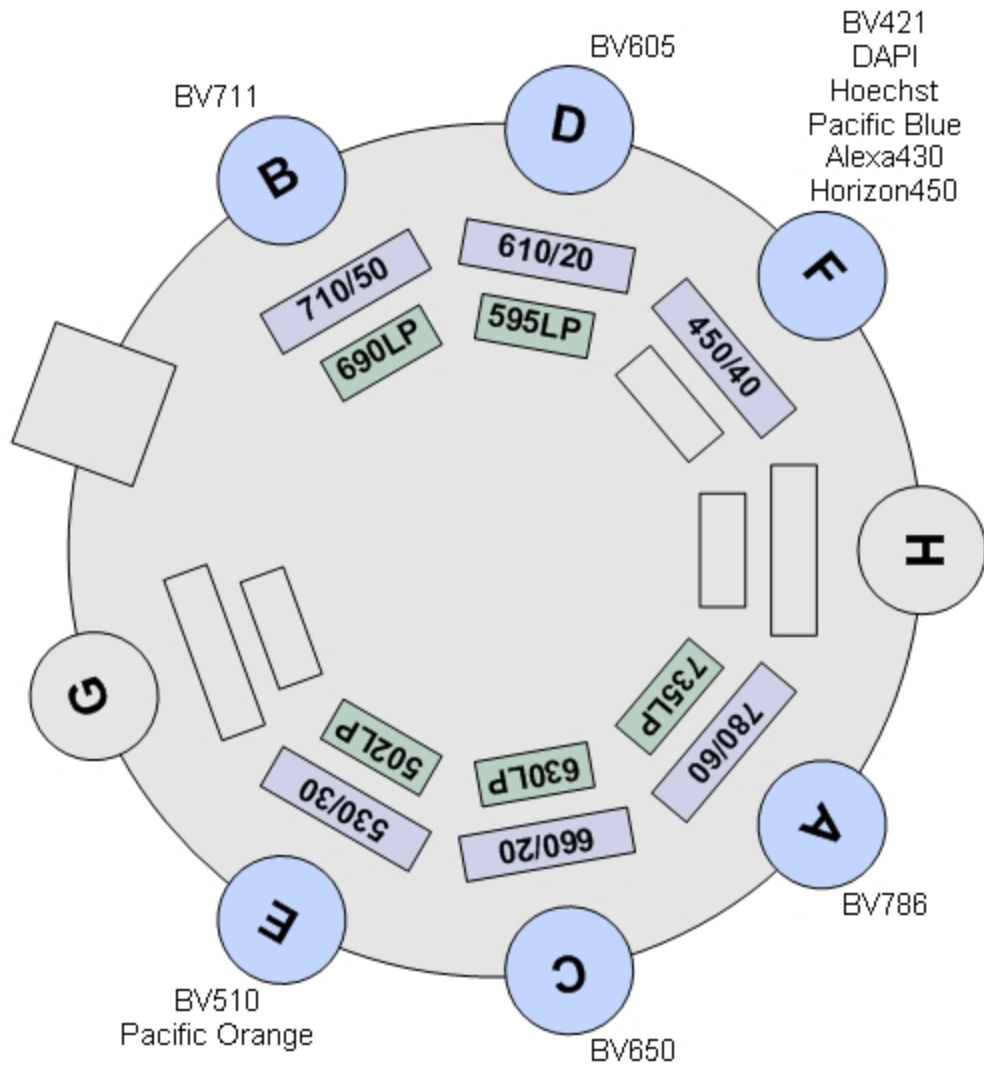

Comments: